

GP33
1-8

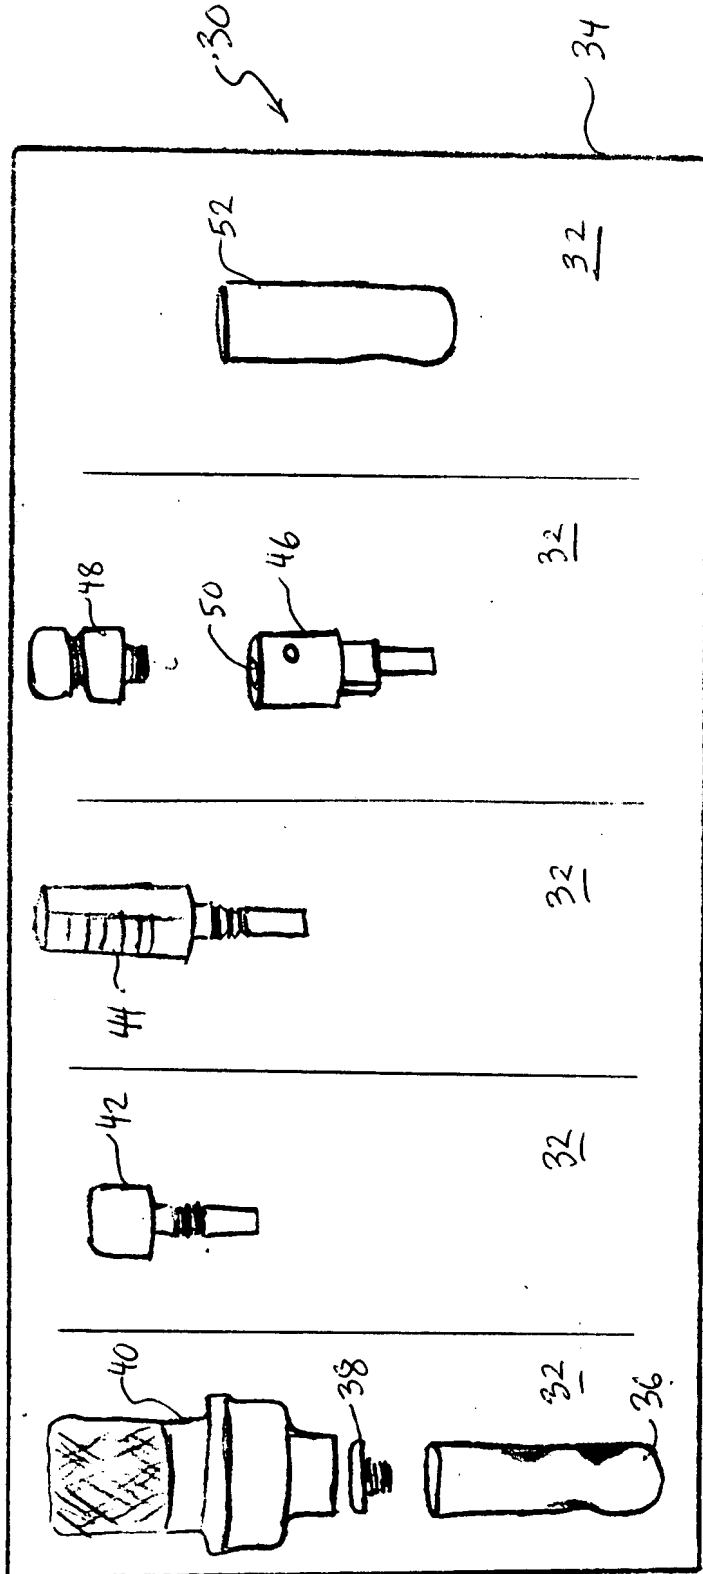


FIGURE 1

Handwritten signature and date:
C. J. P. 11-15-15



FIG. 2

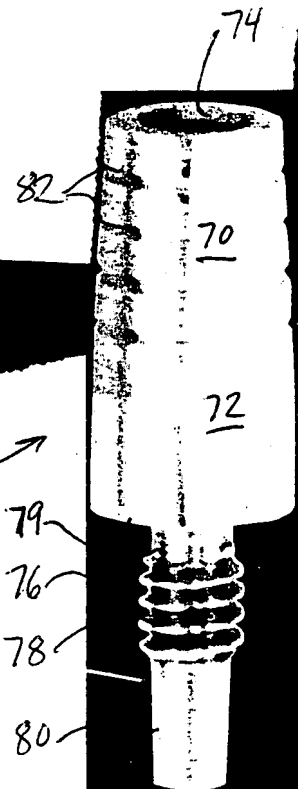
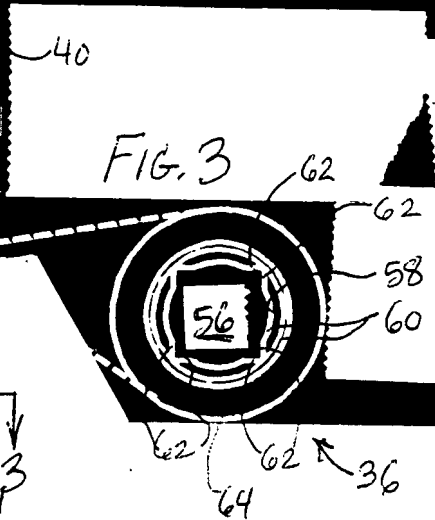


FIG. 4

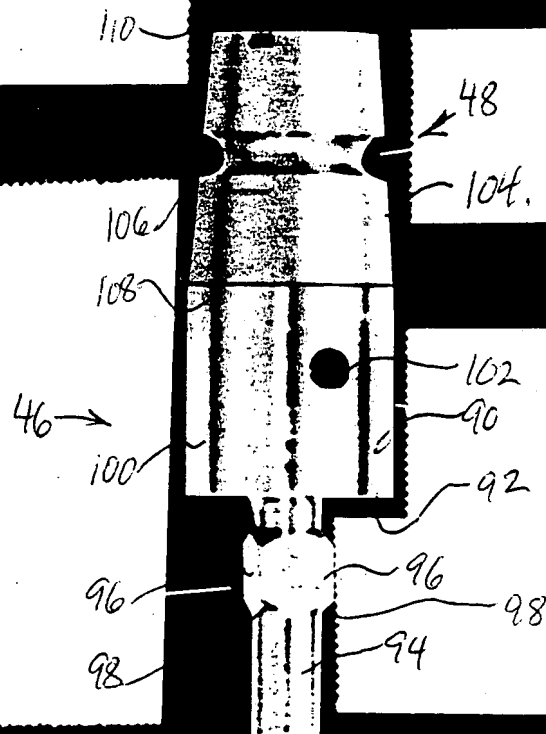


FIG. 5





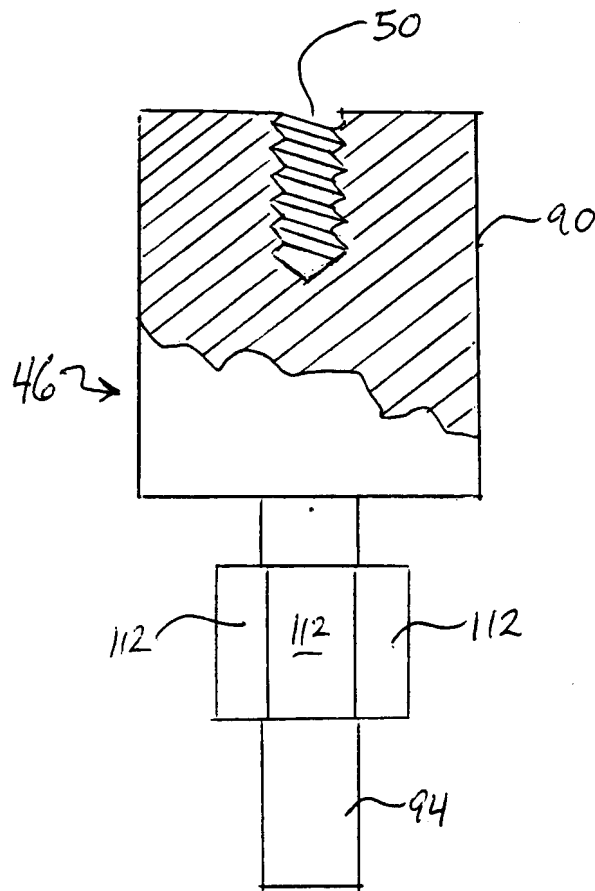


FIGURE 6

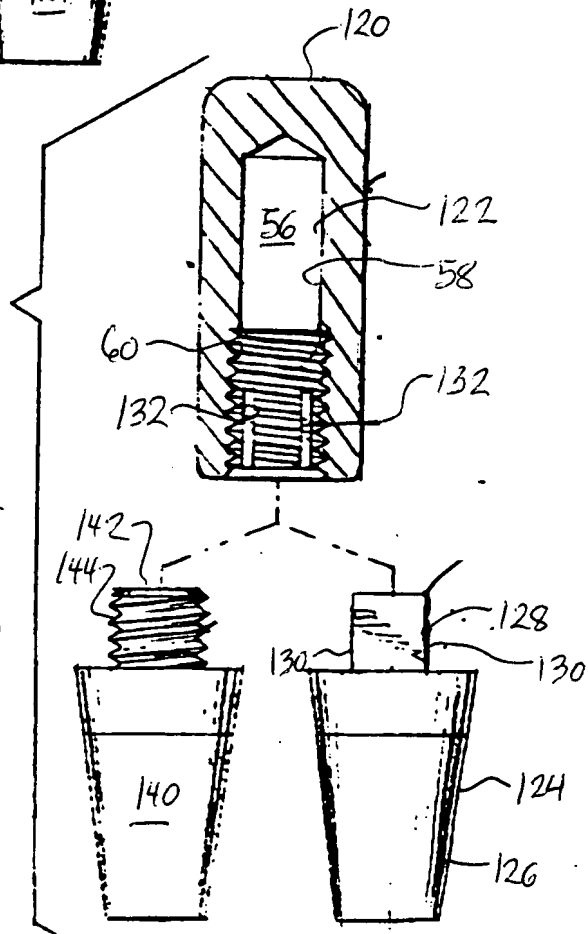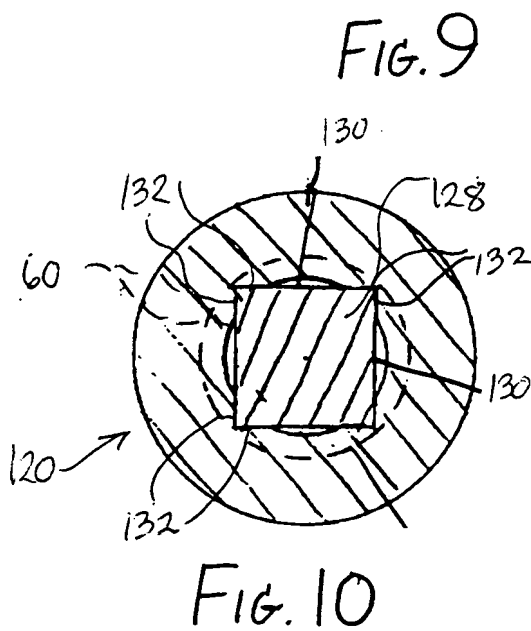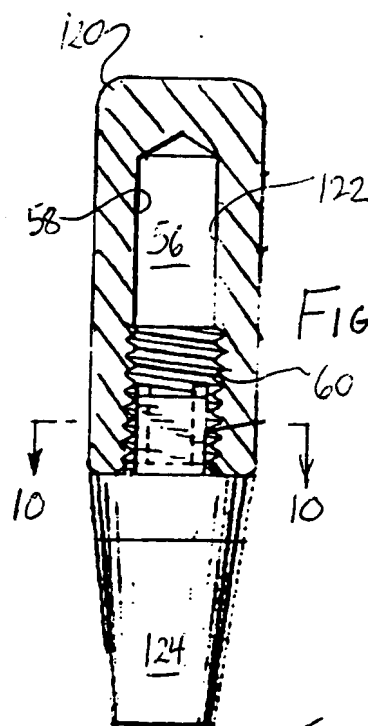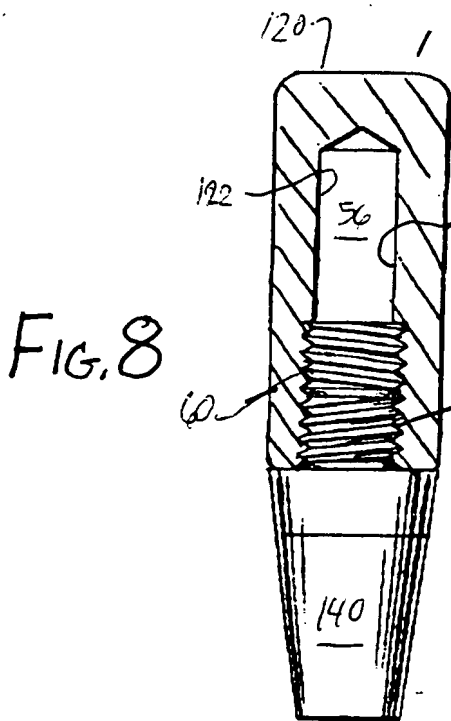

difference in
press fit
in implant body
vs. press fit
attachment mod
70 7 24 4222

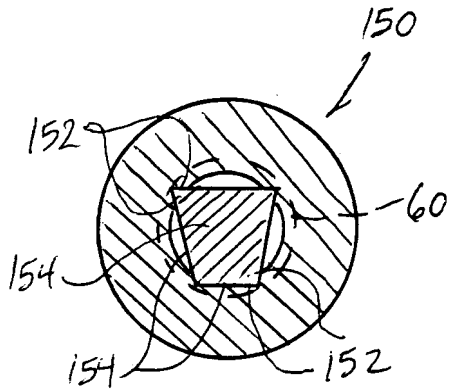


FIG. 11

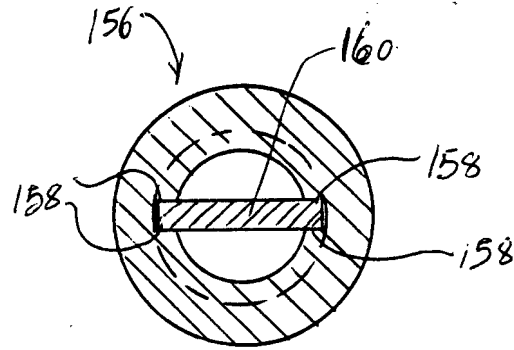


FIG. 12

39184-III
SHEET 6 OF 8

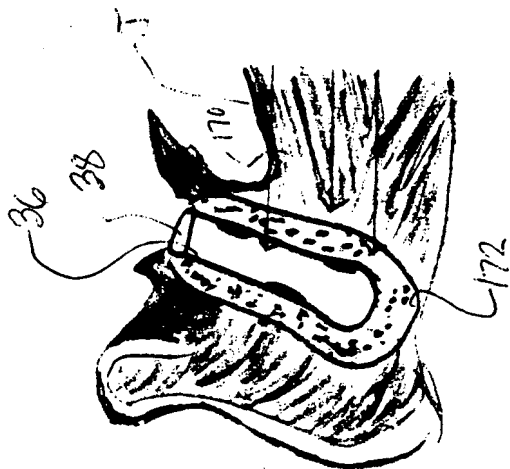


FIGURE 13

blab
4/20/55

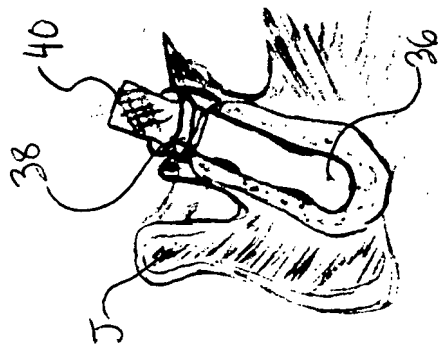


FIG. 14

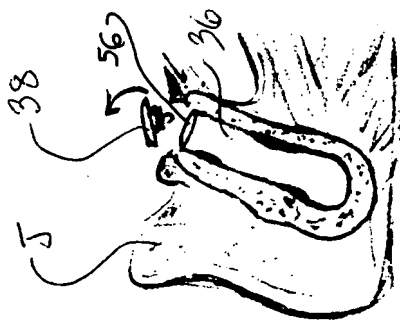


FIG. 15

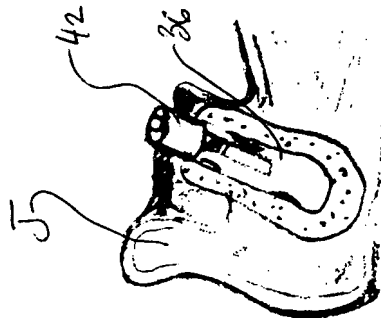


FIG. 16

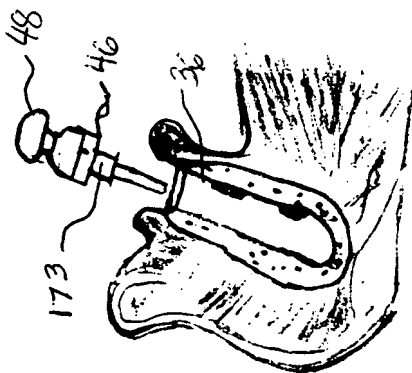


FIG. 17

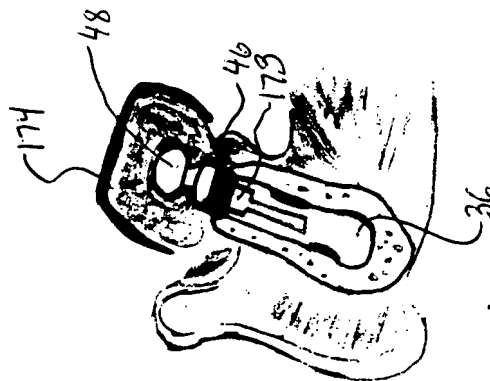


FIG. 18

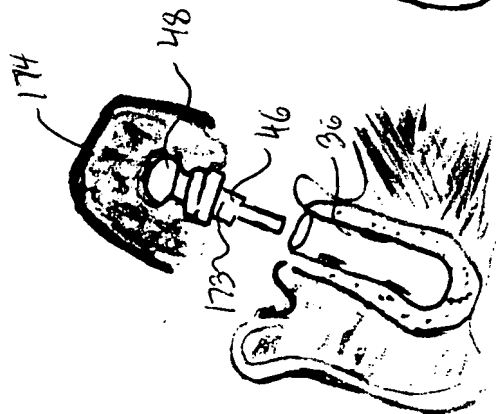


FIG. 19

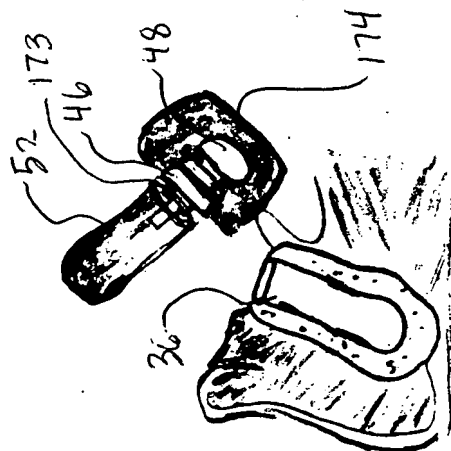


FIG. 20

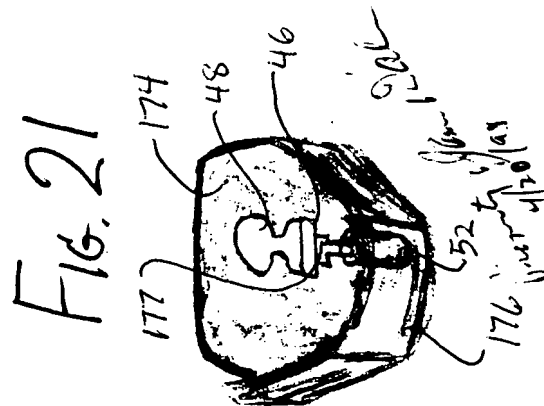


FIG. 21

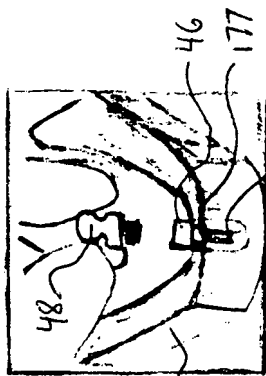


FIG. 22

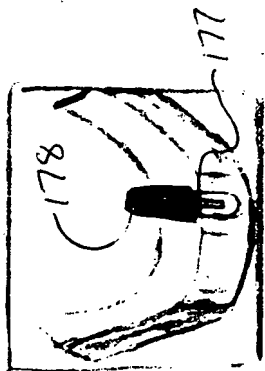


FIG. 23

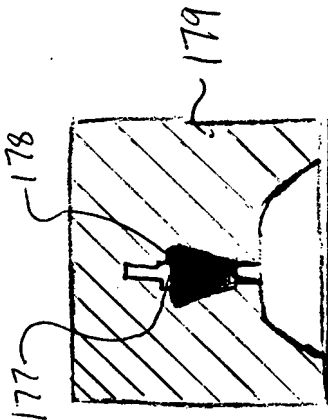


FIG. 24

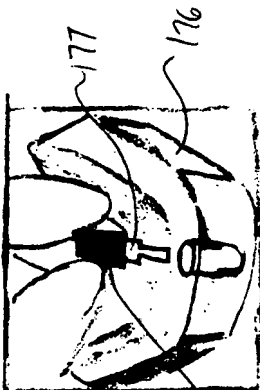


FIG. 25

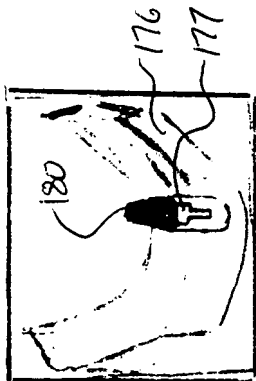


FIG. 26

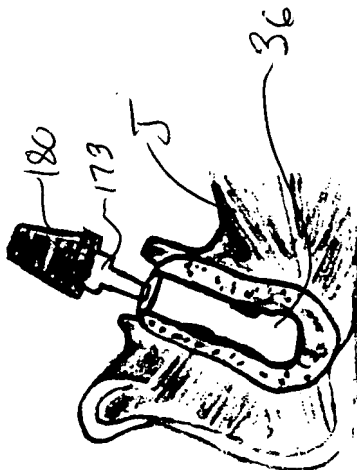


FIG. 27

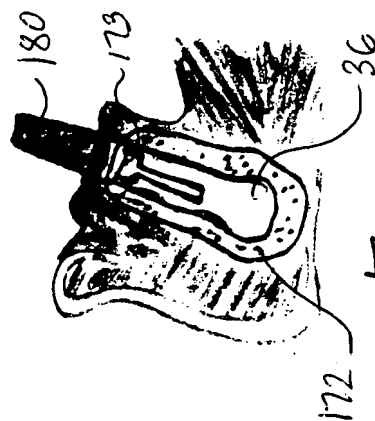


FIG. 28

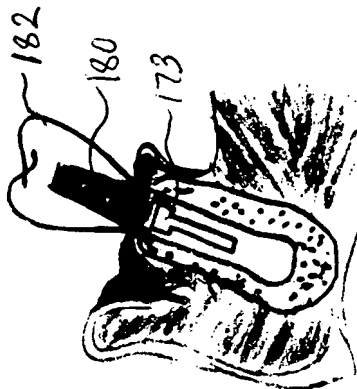


FIG. 29

Continued from Sheet 7 of 8